



METER  
ENVIRONMENT

## CORRECTING TEMPERATURE SENSITIVITY OF ECH<sub>2</sub>O SOIL MOISTURE SENSORS

### INTRODUCTION

In many natural and engineered soils, the output of ECH<sub>2</sub>O soil moisture sensors are sensitive to variations in the soil temperature. The temperature sensitivity is not caused by the ECH<sub>2</sub>O sensors themselves, which are almost perfectly insensitive to temperature changes, but rather the electrical characteristics of the soil, which can be quite sensitive to temperature changes. The ECH<sub>2</sub>O sensors measure volumetric water content (VWC) by measuring the dielectric permittivity ( $\epsilon$ ) of the bulk soil.  $\epsilon$  in the soil is a complex quantity with both real ( $\epsilon'$ ) and imaginary ( $\epsilon''$ ) components.  $\epsilon'$  is the real dielectric permittivity of the soil constituents and has a negative correlation with temperature.  $\epsilon''$  is related to dielectric losses, and more importantly, electrical conduction through the soil.

The ability of a soil to conduct electrical current or electrical conductivity (EC) is related to VWC and the amount of free ions in the soil (solute content). The EC of a soil has a strong positive correlation to temperature. The opposing temperature sensitivities of the real and imaginary components of the dielectric permittivity can be thought of as opposing forces in the soil. In some soils,  $\epsilon'$  dominates, and an increase in temperature causes a decrease in the VWC measured by the ECH<sub>2</sub>O sensor. In other soils,  $\epsilon''$  dominates, and an increase in temperature causes an increase in the VWC measured by the ECH<sub>2</sub>O sensor. In some soils, the two components closely balance each other, and there is no apparent temperature sensitivity in the VWC measurement. Because of these complex interactions, it is impossible to determine a generic correction factor for temperature that can be applied to all soils.

The older ECH<sub>2</sub>O sensors (EC-10 and EC-20) operate at a low measurement frequency and are more strongly affected by  $\epsilon''$ , meaning that there is often a positive relationship between temperature and measured VWC. The new generation of ECH<sub>2</sub>O sensors (EC-5, 5TM, 5TE) operate at a much higher measurement frequency and are much less affected by salts in the soil ( $\epsilon''$ ). With these sensors, the temperature sensitivity is generally small and can be either negative or positive. It should be

noted that any ECH<sub>2</sub>O sensor buried at a depth of more than about 15 cm in the soil, or under a full vegetative canopy, will have little or no noticeable temperature sensitivity due to the very small diurnal fluctuations in soil temperature at these depths or under a closed canopy.

The three strategies described below for correcting the temperature sensitivity of ECH<sub>2</sub>O sensors are meant primarily for users who have sensors placed in the top 15 cm of the soil profile under a bare surface, or whose sensors otherwise undergo strong temperature cycling.

## STRATEGY 1: MULTIPLE REGRESSION ANALYSIS

If temperature data are available at the same location as the ECH<sub>2</sub>O sensor (i.e., 5TM or 5TE sensor), then a multiple regression strategy can be used to relate the true VWC to the measured VWC and temperature data. The general goal is to construct a mathematical model (equation) of the form

$$VWC_{corrected} = C1 * VWC_{meas} + C2 * T_{soil} + C3$$

Where  $VWC_{meas}$  is the VWC measured by the ECH<sub>2</sub>O sensor,  $T_{soil}$  is the soil temperature at the location of the sensor, and C1 – C3 are empirical coefficients determined by multiple regression on field data. The steps below describe how to use the regression tool in Excel and co-located ECH<sub>2</sub>O sensor and temperature data to determine the values of C1 – C3 for a particular soil.

## REQUIREMENTS:

The requirement for this method is co-located temperature and ECH<sub>2</sub>O sensor output data in the soil that you wish to construct the correction model for. The data must have at least two (preferably three or more) 24-hour periods with no rain or irrigation events. For maximum effectiveness, the chosen 24-hour periods should have different average VWC that span the range from wet soil to dry soil (i.e., one 24-hour period with dry soil, one with moderately wet soil, and one with quite wet soil).

## METHOD:

1. Identify three or more 24-hour periods to include in the data analysis (see Figure 1 for example). These periods should meet the following qualifiers:

- 1.1. no precipitation or irrigation in each 24-hour period
- 1.2. group of 24-hour periods spans the range of expected VWC
- 1.3. temperatures at beginning and end of 24-hour period are comparable
- 1.4. no anomalies present in the selected data

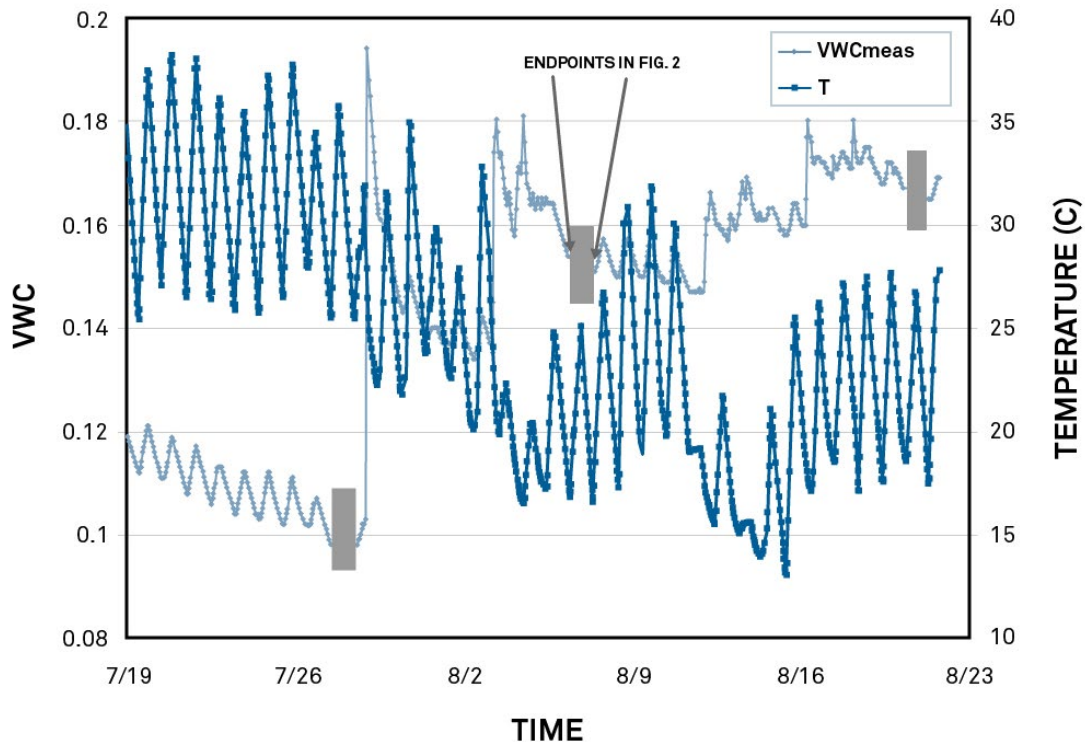


Figure 1. Example of three 24-hour periods chosen from a data set (shown under shaded boxes). The endpoints used for the linear interpolation example data shown in Figure 2 are indicated.

2. Interpolate VWC data between endpoints. To determine the non-temperature affected VWC of the soil during each 24-hour period, constant drainage/evaporation is assumed over the period, and VWC is interpolated as a straight line between the two endpoints of each 24-hour period. This is easily accomplished in Excel by plotting the VWC at the two endpoints on the Y-axis against time on the X-axis. Then, use the trendline function to draw the regression line between them (see Figure 2). The resulting linear equation is then applied to all of the time data in that 24-hour period to interpolate between the two endpoints. Often it is easiest to assign an arbitrary time scale to the data for this part of the correction instead of the time stamp your data acquisition system outputs. For example, if you are collecting data at 30-minute intervals, you would assign X-axis values of 1 to 49 during the interpolation routine, or values of 1 to 25 for hourly data (column A in Table 1). Note

that this process must be repeated for each of the 24-hour periods.

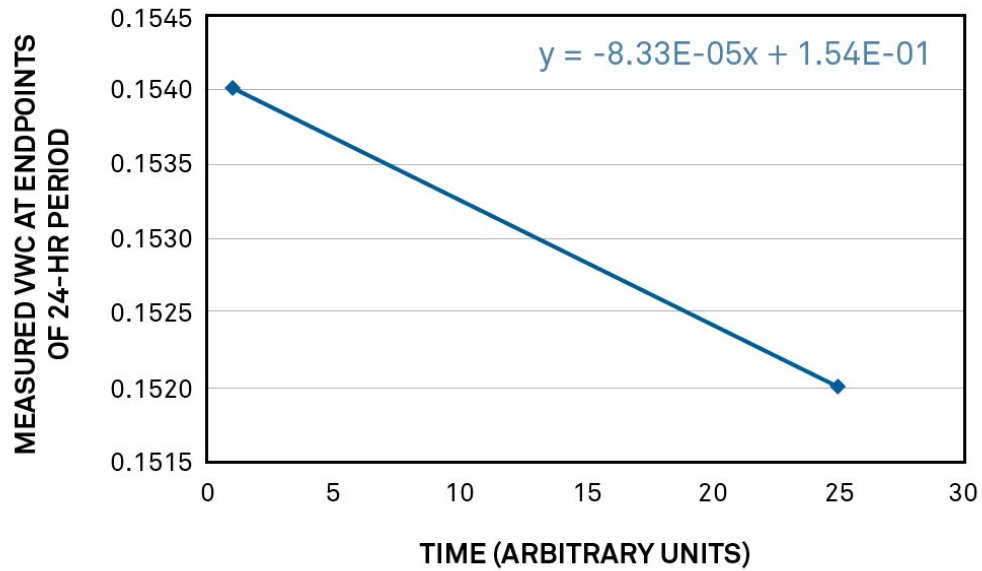


Figure 2. Linear interpolation between two endpoints of one 24-hour period (indicated in Figure 1). The X-axis is column A from Table 1, and the Y-axis is column E from Table 1. The linear equation was generated using the trendline function.

	A	B	C	D	E	F
1	Timescale for Interpolation	Time	VWCmeas	T	VWC for Interpolation	Interpolated VWC
2	1	8/6/2006 11:00	0.154	17.36	0.154	0.154
3	2	8/6/2006 12:00	0.155	18.93		$=-0.0000833*A3+0.154$
4	3	8/6/2006 13:00	0.155	19.74		0.154
5	4	8/6/2006 14:00	0.155	19.93		0.154
6	5	8/6/2006 15:00	0.156	20.77		0.154
7	6	8/6/2006 16:00	0.156	21.87		0.154
8	7	8/6/2006 17:00	0.157	23.11		0.153
9	8	8/6/2006 18:00	0.157	24.41		0.153

10	9	8/6/2006 19:00	0.157	25.01		0.153
11	10	8/6/2006 20:00	0.157	24.14		0.153
12	11	8/6/2006 21:00	0.156	23.26		0.153
13	12	8/6/2006 22:00	0.155	22.44		0.153
14	13	8/6/2006 23:00	0.154	21.58		0.153
15	14	8/7/2006 0:00	0.154	20.83		0.153
16	15	8/7/2006 1:00	0.154	20.16		0.153
17	16	8/7/2006 2:00	0.154	19.61		0.153
18	17	8/7/2006 3:00	0.153	19.03		0.153
19	18	8/7/2006 4:00	0.153	18.42		0.153
20	19	8/7/2006 5:00	0.152	17.87		0.152
21	20	8/7/2006 6:00	0.152	17.47		0.152
22	21	8/7/2006 7:00	0.151	17.07		0.152
23	22	8/7/2006 8:00	0.151	16.68		0.152
24	23	8/7/2006 9:00	0.151	16.45		0.152
25	24	8/7/2006 10:00	0.151	16.57		0.152
26	25	8/7/2006 11:00	0.152	17.27	0.152	0.152

**Table 1.** Example of linear interpolation for a single 24-hour period. Note that the formula shown in cell F3 comes from the linear regression equation from Figure 2, and is applied to cells F3 to F25. Also note the arbitrary time scale in column A. This is often much easier to work with than the timestamp data from many data acquisition systems.

3. Combine all 24-hour periods and run a multiple regression. In Excel, this is easiest accomplished by pasting data from all 24-hour periods into the same columns (see Table 2). Then run the regression tool: Tools>Data Analysis>Regression. Select the interpolated VWC column from step 2 as the Y-variable (C2:C76 in Table 2), and measured VWC and Temperature as your X-axis variables (A2:B76 in Table 2). The regression tool will output several descriptive statistics and the multiple regression coefficients (see Table 3). The coefficients X Variable 1 and X Variable 2 are C1 and C2 in Equation 1 above, and the Intercept is C3. Note that X Variable 1 is the coefficient for the first (leftmost) column of the X-axis variable range (in this case measured VWC).

	A	B	C
1	VWCmeas	T	Interpolated VWC
2	0.098	25.42	0.0979583
3	0.099	25.63	0.0979166
4	0.099	26.87	0.0978749
5	0.1	28.58	0.0978332
6	0.102	30.43	0.0977915
7	0.103	32.27	0.0977498
8	0.105	33.92	0.0977081
9	0.106	35.23	0.0976664
10	0.106	35.64	0.0976247
11	0.106	35.64	0.097583
12	0.107	35.68	0.0975413
13	0.106	35.25	0.0974996
14	0.105	34.39	0.0974579
15	0.104	33.39	0.0974162

16	0.103	32.4	0.0973745
17	0.102	31.51	0.0973328
18	0.102	30.67	0.0972911
19	0.101	29.95	0.0972494
20	0.1	29.14	0.0972077
21	0.099	28.28	0.097166
22	0.099	27.43	0.0971243
23	0.099	26.67	0.0970826
24	0.098	26.03	0.0970409
25	0.097	25.59	0.0969992
26	0.097	25.41	0.0969575
27	0.154	17.36	0.1539167
28	0.155	18.93	0.1538334
29	0.155	19.74	0.1537501
30	0.155	19.93	0.1536668
31	0.156	20.77	0.1535835
32	0.156	21.87	0.1535002
33	0.157	23.11	0.1534169
34	0.157	24.41	0.1533336
35	0.157	25.01	0.1532503
36	0.157	24.14	0.153167
37	0.156	23.26	0.1530837

38	0.155	22.44	0.1530004
39	0.154	21.58	0.1529171
40	0.154	20.83	0.1528338
41	0.154	20.16	0.1527505
42	0.154	19.61	0.1526672
43	0.153	19.03	0.1525839
44	0.153	18.42	0.1525006
45	0.152	17.87	0.1524173
46	0.152	17.47	0.152334
47	0.151	17.07	0.1522507
48	0.151	16.68	0.1521674
49	0.151	16.45	0.1520841
50	0.151	16.57	0.1520008
51	0.152	17.27	0.1519175
52	0.167	19.54	0.1669583
53	0.168	21.14	0.1669166
54	0.168	22.31	0.1668749
55	0.169	23.54	0.1668332
56	0.169	25	0.1667915
57	0.17	26.17	0.1667498
58	0.17	26.65	0.1667081
59	0.17	26.51	0.1666664



60	0.17	25.83	0.1666247
61	0.169	24.91	0.166583
62	0.169	23.84	0.1665413
63	0.168	22.84	0.1664996
64	0.168	21.99	0.1664579
65	0.167	21.33	0.1664162
66	0.167	20.54	0.1663745
67	0.166	19.76	0.1663328
68	0.166	19.07	0.1662911
69	0.166	18.51	0.1662494
70	0.165	18.09	0.1662077
71	0.165	17.66	0.166166
72	0.165	17.44	0.1661243
73	0.165	17.42	0.1660826
74	0.165	17.65	0.1660409
75	0.165	18.3	0.1659992
76	0.166	19.56	0.1659575

**Table 2.** Combined data from three 24-hour periods, ready for multiple regression. With all 24-hour periods in the same columns, the multiple regression analysis will include data from all three days.

## Regression Statistics

Multiple R	0.99954768
R Square	0.999095565
Adjusted R Square	0.999070442
Standard Error	0.000916358
Observations	75

Table 3. Summary output

	df	SS	MS	F	Significance F
Regression	2	0.06678705	0.033393525	39767.8662	2.6889E-110
Residual	72	6.04592E-05	8.39711E-07		
Total	74	0.066847509			

Table 4. ANOVA

	Coefficient	Standard Error	t Stat	P-value	Lower 95%	Upper 95%
Intercept	0.016239203	0.001353677	11.99636264	7.70761E-19	0.013540697	0.018937709
X Variable 1	0.965494597	0.005510463	175.2111411	1.83299E-96	0.954509689	0.976479505
X Variable 2	-0.000562114	2.79704E-05	-20.09677639	3.02271E-31	-0.000617872	-0.000506356

Table 5. Example output from Excel regression function. Shaded cells contain the information important for this analysis.

4. Construct a VWC correction model. Use the coefficients determined from the multiple regression in part 3 to construct a VWC correction model from Equation 1. In the case of the example data, the model would be

$$VWC_{corrected} = 0.9655 * VWC_{meas} - 5.621 \times 10^{-4} * T_{soil} + 1.624 \times 10^{-2}$$

Equation 2

5. Apply the model to your raw data set, yielding corrected VWC. The temperature dependency in the corrected VWC data should be greatly reduced. In some instances, there will still be some apparent temperature dependence. Often the results can be improved by selecting data to input into the correction algorithm that more fully span the range of VWC encountered in the soil.

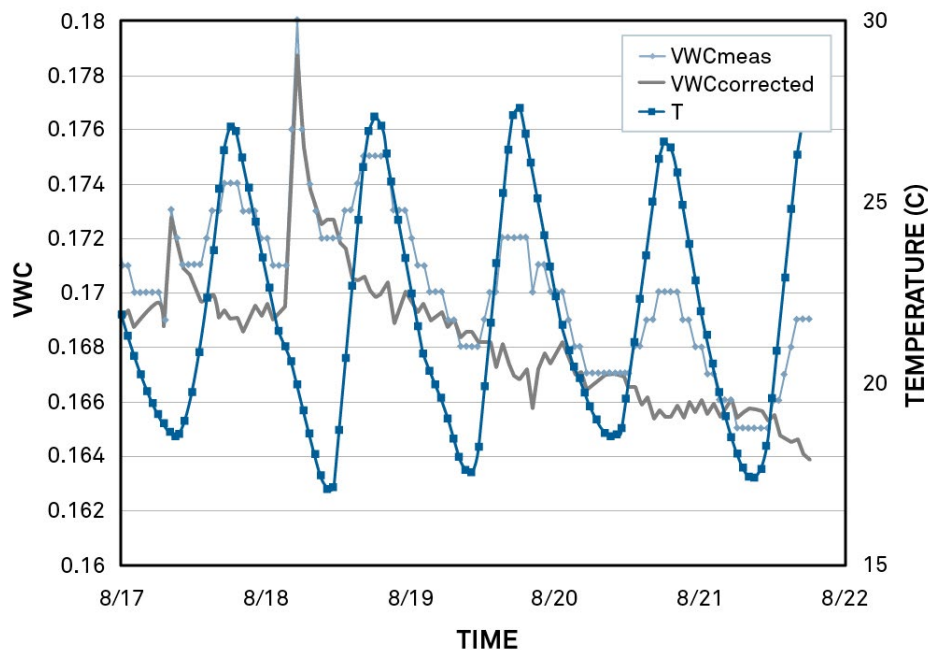


Figure 3. Example of temperature-corrected data. Notice that with this method the VWC dynamics are preserved, but the temperature dependency is greatly reduced compared to the uncorrected data.

## STRATEGY 2: ONCE-PER-DAY MEASUREMENTS OR AVERAGING

Soil moisture is reasonably conservative and does not change much in a day unless a precipitation or [irrigation](#) event occurs. So, if no temperature information is available, or if a simplified smoothing technique is preferred, using once-per-day water content measurement or designing a simple averaging technique is useful. Of course, this would wash out any hourly changes that might be of interest, but in our experience, we generally see very little temperature-related fluctuations in the [water content data](#) when there are multiple rain or irrigation events during a day, so these data would not need correction.

Implementing a once-per-day strategy involves selecting a time to use, culling and sorting the data, and checking to make sure the results fit the original data satisfactorily. We have chosen early morning hours (e.g., 2 AM) where temperature

is near its minimum as our daily measurement. This reduces the likelihood of variation in the soil moisture data from changing daily high temperatures. To sort a dataset for 2 AM data, we use an “if” statement in Excel that only puts data into an adjoining column when it is 2 AM (Table 3). Once you have set up the formula for your worksheet, copy and paste so it covers all the date values and any water content columns you want to include. Next, use the sort command to collapse all the spaces in the data and sort your data by date. You should be left with a fraction of your original data that you can now graph against the full data to see the fit. Figure 4 shows that this method does a good job smoothing the data. Obviously, this technique will not preserve the high-frequency soil moisture dynamics, but the overall trends in soil moisture will remain.

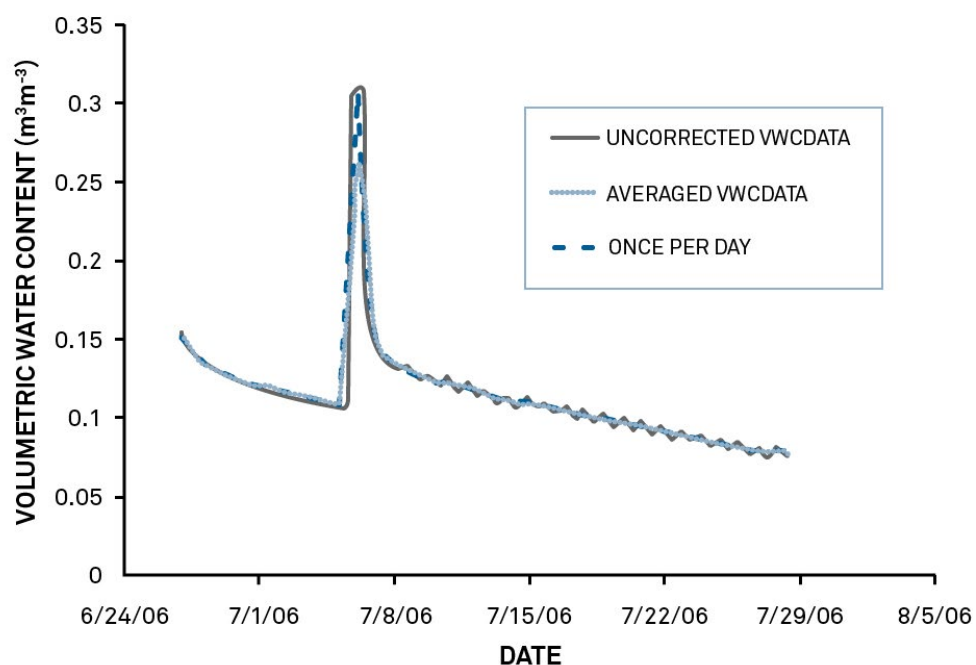


Figure 4. Once-per-day smoothing and averaging of water content data. Original data courtesy of S. Tyler, J. Selker, and S. Assouline.

Data averaging is another way that you can smooth temperature cycling in the water content data. The advantage of this technique is that you can use the entire dataset instead of removing all but one reading per day. Implementing this technique is straightforward; simply make a new column for smoothed water content data and select the “Average()” function in Excel. For the data range, you must average an entire 24-hour period to remove the diurnal temperature cycle so the average function range in any given cell must include data from the past 12 hours and the next 12 hours. Data from the averaging are shown in Figure 4. From our analysis, this averaging technique did not appear to give better results than the once-per-day technique and, not surprisingly, tended to smooth large changes in water content.

## STRATEGY 3: A CALIBRATION METHOD USING TIME SERIES OF FIELD DATA THAT REQUIRES NO LABORATORY EXPERIMENTS

See the following paper:

Saito, Tadaomi, Haruyuki Fujimaki, Hiroshi Yasuda, Koji Inosako, and Mitsuhiro Inoue. "Calibration of temperature effect on dielectric probes using time series field data." *Vadose Zone Journal* 12, no. 2 (2013). [Article link](#).

REQUEST A QUOTE

CONTACT US